



ClientFuturistic Science LLC

Analyzed08/18/2026

This Certificate of Analysis certifies that the sample listed herein was tested by SteriGenix using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

Product	Acetic Acid	Form	Liquid
Batch	FS-AACID-3ML-0926	Labeled Qty	3mL
Mol. Formula	CH3COOH	CAS Number	64-19-7
Cap Color	White	Crimp Color	Silver
Appearance	Clear		

TEST RESULTS

	REFERENCE STANDARD	RESULT	
Identity Confirmation (LC-MS)	Acetic Acid	Matches	✓
Batch Avg Purity (HPLC)	(>98%)	99.57%	✓
Net Content	± 10%	2.98mL	✓
Sterility	Bacterial Growth (Accelerator)	No Growth	✓

HEAVY METAL SCREENING


No data.

BATCH CONFORMITY RESULTS

No data.

HPLC CHROMATOGRAM

HPLC CHROMATOGRAM · ACETIC ACID	DETECTOR: UV 214 NM · 08/18/2026

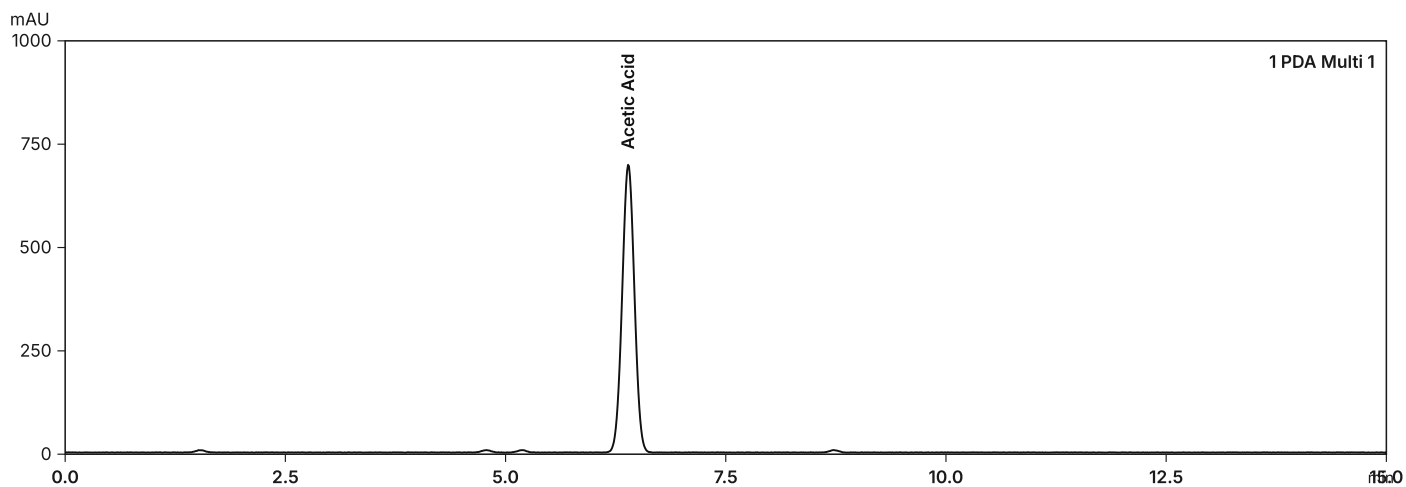

SAMPLE PHOTOS



AS RECEIVED

RECONSTITUTED (BACT. WATER) — CLARITY
CHECK

Dr. R. Caldwell

ANALYST
ID: AN-3271

Dr. P. Andersen

QC REVIEWER
ID: QR-5418

Dr. H. Whitman

QA DIRECTOR
ID: QA-1090



sterigenixanalytical.com/verify

Report#: RPT-2026-640001
Access Code: SGX-FS-2026-0810-B82

